



Swansea University
Prifysgol Abertawe



Cronfa - Swansea University Open Access Repository

This is an author produced version of a paper published in:
Surface Science Spectra

Cronfa URL for this paper:
<http://cronfa.swan.ac.uk/Record/cronfa46101>

Paper:

Jones, D., Warwick, M., McGettrick, J. & Dunnill, C. (2018). Composition analysis of Ta₃N₅/W₁₈O₄₉ nanocomposite through XPS. *Surface Science Spectra*, 25(2), 024002
<http://dx.doi.org/10.1116/1.5047860>

This item is brought to you by Swansea University. Any person downloading material is agreeing to abide by the terms of the repository licence. Copies of full text items may be used or reproduced in any format or medium, without prior permission for personal research or study, educational or non-commercial purposes only. The copyright for any work remains with the original author unless otherwise specified. The full-text must not be sold in any format or medium without the formal permission of the copyright holder.

Permission for multiple reproductions should be obtained from the original author.

Authors are personally responsible for adhering to copyright and publisher restrictions when uploading content to the repository.

<http://www.swansea.ac.uk/library/researchsupport/ris-support/>

Composition analysis of Ta₃N₅/W₁₈O₄₉ nanocomposite through XPS

Daniel R. Jones, Michael E. A. Warwick, James D. McGettrick, and Charles W. Dunnill

Citation: *Surface Science Spectra* **25**, 024002 (2018); doi: 10.1116/1.5047860

View online: <https://doi.org/10.1116/1.5047860>

View Table of Contents: <http://avs.scitation.org/toc/sss/25/2>

Published by the [American Vacuum Society](#)



Instruments for Advanced Science

Contact Hiden Analytical for further details:

W www.HidenAnalytical.com

E info@hiden.co.uk

CLICK TO VIEW our product catalogue



Gas Analysis

- › dynamic measurement of reaction gas streams
- › catalysis and thermal analysis
- › molecular beam studies
- › dissolved species probes
- › fermentation, environmental and ecological studies




Surface Science

- › UHV TPD
- › SIMS
- › end point detection in ion beam etch
- › elemental imaging - surface mapping



Plasma Diagnostics

- › plasma source characterization
- › etch and deposition process reaction
- › kinetic studies
- › analysis of neutral and radical species



Vacuum Analysis

- › partial pressure measurement and control of process gases
- › reactive sputter process control
- › vacuum diagnostics
- › vacuum coating process monitoring

Composition analysis of Ta₃N₅/W₁₈O₄₉ nanocomposite through XPS

Daniel R. Jones,¹ Michael E. A. Warwick,¹ James D. McGettrick,² and Charles W. Dunnill^{1,a)}

¹*Energy Safety Research Institute (ESRI), Swansea University Bay Campus, Swansea SA1 8EN, United Kingdom*

²*SPECIFIC Swansea University Bay Campus, Swansea SA1 8EN, United Kingdom*

(Received 10 July 2018; accepted 11 October 2018; published 12 November 2018)

A characterization of a nanocomposite material consisting of Ta₃N₅ nanoparticles and W₁₈O₄₉ nanowires is presented. The material is of interest for photocatalytic applications, with a focus on pollution reduction through the photodegradation of dye waste; under white light illumination, the combination of Ta₃N₅ and W₁₈O₄₉ yielded an enhanced rate of dye degradation relative to Ta₃N₅ particles alone. The facile method of synthesis is thought to be a promising route for both upscale and commercial utilization of the material. X-ray photoelectron spectroscopy revealed a core-shell composite structure with W₁₈O₄₉ present as an overlayer on Ta₃N₅; the analyzed spectra for the C 1s, O 1s, Ta 4f, N 1s, W 4f, and Na 1s regions are reported. It should be noted that due to differential charging of the underlying Ta₃N₅ component relative to the W₁₈O₄₉ shell, an additional uncompensated voltage shift may exist in the Ta 4f and N 1s spectra. *Published by the AVS.*

<https://doi.org/10.1116/1.5047860>

Keywords: Ta₃N₅, W₁₈O₄₉, photocatalysis, dye degradation, composite, nanowires, x-ray photoelectron spectroscopy, XPS

INTRODUCTION

Many synthetic dyes are toxic to both human (Ref. 1) and marine life (Ref. 2) and inhibit aquatic photosynthesis through light absorption (Ref. 3), leading to concerns for global oxygen production. Many synthetic dyes are, by design, chemically stable and are therefore difficult to degrade via common biological treatment (Refs. 4 and 5), while alternative techniques can lead to the production of unwanted by-products which are also harmful (Refs. 6–9). One promising, low-energy solution for the remediation of dye-polluted water is the use of photocatalysts for oxidation of the dyes. Much work has focused on the use of TiO₂ nanopowders for this purpose (Refs. 10–17); however, TiO₂ has a wide bandgap (3.2 eV) and can therefore utilize only the ultraviolet portion of the solar spectrum, which accounts for a small percentage of solar radiation that reaches the earth. With this in mind, it is preferable to employ a material with a narrower bandgap so that dye oxidation may be instigated by visible light. With its low bandgap of 2.1 eV (Ref. 18), Ta₃N₅ has been shown to work well as a visible light photocatalyst for the degradation of organic dyes (Refs. 19–21), although our recent study demonstrated how the catalytic performance of this material may be enhanced through a strategic combination with tungsten(IV) suboxide nanowires in the form of a composite (Ref. 22). Within this investigation, a solvothermal approach was employed to grow W₁₈O₄₉ nanofibers on Ta₃N₅ nanoparticles inside a polytetrafluoroethylene-lined stainless steel acid digestion bomb, and it was found that the combination of these materials resulted in improved charge carrier separation due to electron-hole transfer at the interface of the two components; the increase in charge separation afforded longer charge carrier lifetimes, resulting in a marked increase in the photocatalytic activity of the material. To the

best of the authors' knowledge, this system has not before been synthesized for the purpose of water remediation.

SPECIMEN DESCRIPTION (ACCESSION #01477)

Host Material: Ta₃N₅/W₁₈O₄₉ nanocomposite

CAS Registry #: Unknown

Host Material Characteristics: Inhomogeneous; powder; polycrystalline; semiconductor; composite

Chemical Name: Tantalum(V) nitride/tungsten(VI) suboxide

Source: Solvothermally grown W₁₈O₄₉ on Ta₃N₅ from ammonolyzed TaCl₅

Host Composition: Ta₃N₅/W₁₈O₄₉

Form: Polycrystalline composite

Structure: Orthorhombic Ta₃N₅/monoclinic W₁₈O₄₉

History and Significance: Ta₃N₅ nanoparticles were prepared through ammonolysis of TaCl₅ powder in a 7:3 molar ratio of KCl and NaCl at 800 °C for 10 h. Nanowires of W₁₈O₄₉ were subsequently grown solvothermally on the surface of the Ta₃N₅ nanoparticles by annealing a suspension of the nanoparticles in a solution of WCl₆ in a 4:1 volumetric mixture of ethanol and ethylene glycol at 180 °C for 24 h, followed by centrifugation of the product in ethanol and deionized water.

As Received Condition: The as-synthesized composite had the form of a brown powder.

Analyzed Region: Same as the host material

Ex Situ Preparation/Mounting: The composite powder was loaded into a 5 mm pellet press and pelletized using a force of 2 tons. The pellet was retrieved from the press and mounted on an adhesive carbon tab for analysis.

In Situ Preparation: None

^{a)}Electronic mail: c.dunnill@swansea.ac.uk

Charge Control: Electronic charge neutralization using magnetic immersion lens. Filament current = 0.4 A, charge balance = 3.3 V, filament bias = 1.0 V.

Temp. During Analysis: 300 K

Pressure During Analysis: 4×10^{-6} Pa

Preanalysis Beam Exposure: 0 s

INSTRUMENT DESCRIPTION

Manufacturer and Model: Kratos Axis Supra

Analyzer Type: Spherical sector

Detector: Multichannel resistive plate

Number of Detector Elements: 3 MCP, 128 channel DLD

INSTRUMENT PARAMETERS COMMON TO ALL

SPECTRA

■ Spectrometer

Analyzer Mode: Constant pass energy

Throughput ($T = E^N$): $N = 0$

Excitation Source Window: Not specified

Excitation Source: Al K_{α} monochromatic

Source Energy: 1486.6 eV

Source Strength: 225 W

Source Beam Size: $700 \mu\text{m} \times 300 \mu\text{m}$

Signal Mode: Multichannel direct

■ Geometry

Incident Angle: 54.7°

Source-to-Analyzer Angle: 54.7°

Emission Angle: 0°

Specimen Azimuthal Angle: N/A

Acceptance Angle from Analyzer Axis: 0°

Analyzer Angular Acceptance Width: $30^{\circ} \times 30^{\circ}$

■ Ion Gun

Manufacturer and Model: Kratos GCIS Minibeam 6

Energy: 10 keV

Current: 23 nA

Current Measurement Method: Biased stage

Sputtering Species: Argon 1000+ ion clusters

Spot Size (unrastered): $200 \mu\text{m}$

Raster Size: $2000 \mu\text{m} \times 2000 \mu\text{m}$

Incident Angle: 40°

Polar Angle: 0°

Azimuthal Angle: 0°

Comment: Sputtering was carried out on the reference samples only.

DATA ANALYSIS METHOD

Energy Scale Correction: The binding energy scale was referenced to C $1s = 284.8$ eV.

Recommended Energy Scale Shift: 3.213 eV

Peak Shape and Background Method: Peak shape: Gaussian–Lorentzian product formula GL(30). Background: The Shirley background was used.

Quantitation Method: Quantification was achieved through peak deconvolution using CASAXPS version 2.3.15. Relative sensitivity factors were supplied by Kratos Analytical.

ACKNOWLEDGMENTS

Financial support was provided by the Welsh Government Sêr Cymru Programme and the Flexis project, which is part-funded by the European Regional Development Fund (ERDF) through the Welsh Government.

REFERENCES

1. T. Plaztek, C. Lang, G. Grohmann, U.-S. Gi, and W. Baltes, *Hum. Exp. Toxicol.* **18**, 552 (1999).
2. M. Sumathi, K. Kalaiselvi, M. Palanivel, and P. Rajaguru, *Bull. Environ. Contam. Toxicol.* **66**, 407 (2001).
3. O. Gulnaz, *J. Hazard. Mater.* **108**, 183 (2004).
4. A. Srinivasan and T. Viraraghavan, *J. Environ. Manage.* **91**, 1915 (2010).
5. T. Robinson, G. McMullan, R. Marchant, and P. Nigam, *Bioresour. Technol.* **77**, 247 (2001).
6. H. Nourmoradi, S. Zabihollahi, and H. R. Pourzamani, *Desalin. Water Treat.* **57**, 5200 (2015).
7. A. K. Verma, R. R. Dash, and P. Bhunia, *J. Environ. Manage.* **93**, 154 (2012).
8. Y. Li *et al.*, *Chem. Eng. Res. Des.* **91**, 361 (2013).
9. G. Mezohegyi, F. P. van der Zee, J. Font, A. Fortuny, and A. Fabregat, *J. Environ. Manage.* **102**, 148 (2012).
10. A. Ajmal, I. Majeed, R. N. Malik, H. Idriss, and M. A. Nadeem, *RSC Adv.* **4**, 37003 (2014).
11. J. C. Bear, V. Gomez, N. S. Kefallinos, J. D. McGettrick, A. R. Barron, and C. W. Dunnill, *J. Colloid Interf. Sci.* **460**, 29 (2015).
12. V. Gomez, J. C. Bear, P. D. McNaughton, J. D. McGettrick, T. Watson, C. Charbonneau, P. O'Brien, A. R. Barron, and C. W. Dunnill, *Nanoscale* **7**, 17735 (2015).
13. C. W. Dunnill, Z. A. Aiken, J. Pratten, M. Wilson, and I. P. Parkin, *Chem. Vap. Deposition* **16**, 50 (2010).
14. C. W. Dunnill, Z. Ansari, A. Kafizas, S. Perni, D. J. Morgan, M. Wilson, and I. P. Parkin, *J. Mater. Chem.* **21**, 11854 (2011).
15. C. W. Dunnill, S. Noimark, and I. P. Parkin, *Thin Solid Films* **520**, 5516 (2012).
16. M. E. A. Warwick, C. W. Dunnill, and R. Binions, *Chem. Vap. Deposition* **16**, 220 (2010).
17. C. W. Dunnill, K. Page, Z. A. Aiken, S. Noimark, G. Hyett, A. Kafizas, J. Pratten, M. Wilson, and I. P. Parkin, *J. Photochem. Photobiol. A* **220**, 113 (2011).
18. M. Hara, G. Hitoki, T. Takata, J. N. Kondo, H. Kobayashi, and K. Domen, *Catal. Today* **78**, 555 (2003).
19. Z. Wang, J. Hou, S. Jiao, K. Huang, and H. Zhu, *J. Mater. Chem.* **22**, 21972 (2012).
20. D.-H. Lin and K.-S. Chang, *J. Appl. Phys.* **120**, 075303 (2016).
21. S.-T. Bae, H. Shin, S. Lee, D. W. Kim, H. S. Jung, and K. S. Hong, *React. Kinet. Mech. Cat.* **106**, 67 (2011).
22. D. R. Jones *et al.*, *Sci. Rep.* **7**, 4090 (2017).

SPECTRAL FEATURES TABLE

Spectrum ID #	Element/ Transition	Peak Energy (eV)	Peak Width FWHM (eV)	Peak Area (eV × counts/s)	Sensitivity Factor	Concentration (at. %)	Peak Assignment
01477-02	W 4f _{7/2}	35.9	1.14	33 987	3.523	12.84	WO ₃
01477-02	W 4f _{5/2}	38.1	1.14	25 490	3.523	...	WO ₃
01477-02	W 4f _{7/2}	34.6	0.93	4 298	3.523	...	W ₂ O ₅
01477-02	W 4f _{5/2}	36.7	0.93	3 223	3.523	...	W ₂ O ₅
01477-03	O 1s	530.6	1.21	41 006	0.780	40.20	WO ₃ /W ₂ O ₅
01477-03	O 1s	531.6	1.21	8 556	0.780	...	Surface –OH
01477-03	O 1s	532.6	1.21	5 319	0.780	...	Adventitious organics
01477-03	O 1s	533.6	1.21	2 904	0.780	...	Adventitious organics
01477-04	C 1s	284.8	1.35	18 539	0.278	45.52	Adventitious C–C/C–H
01477-04	C 1s	286.4	1.35	2 820	0.278	...	Adventitious C–O/C=O
01477-05	Ta 4f	25.4	0.86	1 731	3.082	0.62	Ta ₃ N ₅
01477-06	N 1s	396.7	0.93	351	0.477	0.81	Ta ₃ N ₅

ANALYZER CALIBRATION TABLE


Spectrum ID #	Element/ Transition	Peak Energy (eV)	Peak Width FWHM (eV)	Peak Area (eV × counts/s)	Sensitivity Factor	Concentration (at. %)	Peak Assignment
08	Ag 3d _{5/2}	368.4	0.51	71 961	5.987	...	Ag
10	Au 4f _{7/2}	84.0	0.60	314 838	6.250	...	Au
12	Cu 2p _{3/2}	933.0	0.80	401 503	5.321	...	Cu

GUIDE TO FIGURES


Spectrum (Accession) #	Spectral Region	Voltage Shift^a	Multiplier	Baseline	Comment #^b
01477-01	Survey	3.213	1	0	1
01477-02	W 4f	3.213	1	0	1
01477-02	W 4f	3.213	1	0	1
01477-03	O 1s	3.213	1	0	1
01477-03	O 1s	3.213	1	0	1
01477-04	C 1s	3.213	1	0	1
01477-04	C 1s	3.213	1	0	1
01477-05	Ta 4f	3.213	1	0	1
01477-06	N 1s	3.213	1	0	1
07	Survey	0	1	0	2
08	Ag 3d _{5/2}	0	1	0	2
09	Survey	0	1	0	3
10	Au 4f _{7/2}	0	1	0	3
11	Survey	0	1	0	4
12	Cu 2p _{3/2}	0	1	0	4

^aVoltage shift of the published figure relative to the as-measured spectrum; the energy correction accounts for the effects of sample charging.

^b1. Ta₃N₅/W₁₈O₄₉ nanocomposite. 2. Ag calibration. 3. Au calibration. 4. Cu calibration.

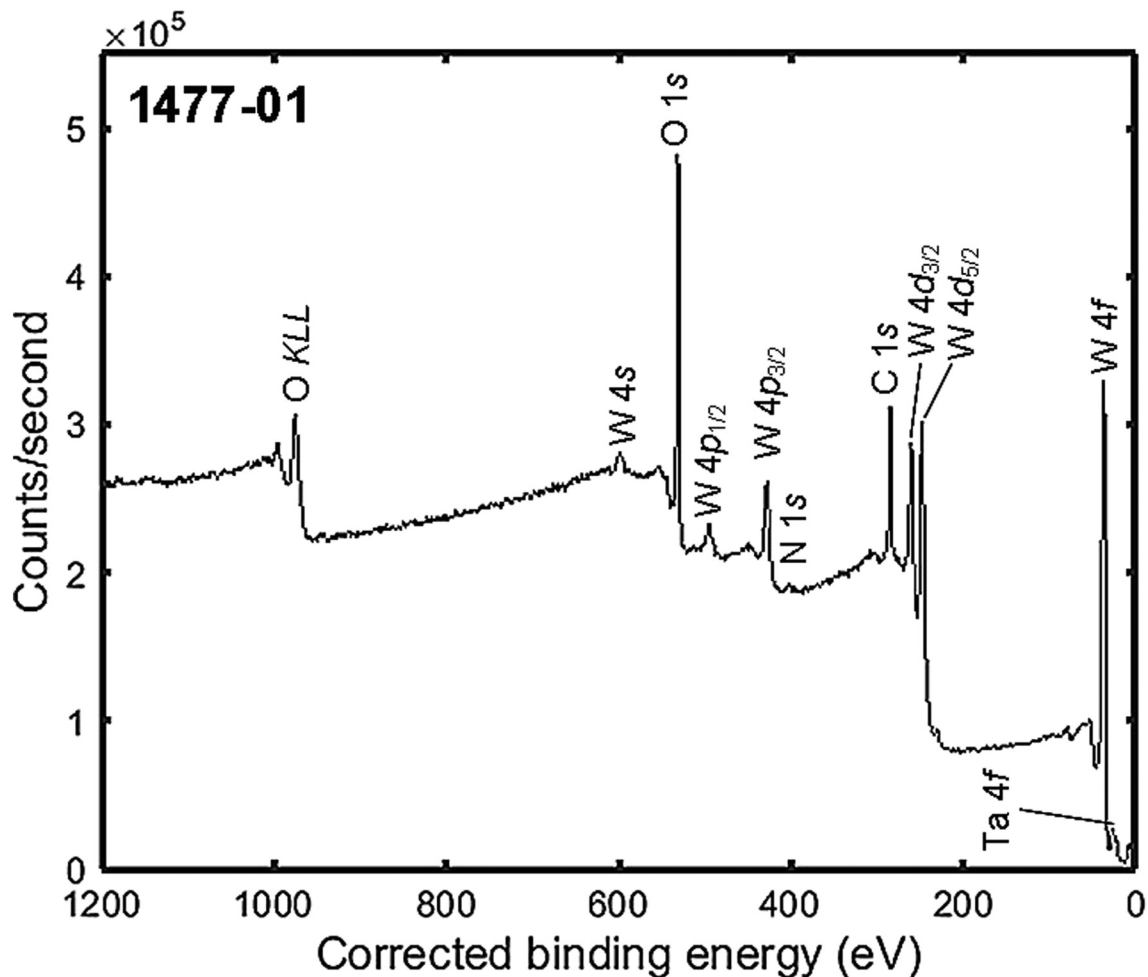


Accession #	01477-01
Host Material:	Ta ₃ N ₅ /W ₁₈ O ₄₉ nanocomposite
Technique:	XPS
Spectral Region:	Survey
Instrument:	Kratos Axis Supra
Excitation Source:	Al K _α monochromatic
Source Energy:	1486.6 eV
Source Strength:	225 W
Source Size:	0.7 mm × 0.3 mm
Analyzer Type:	Spherical sector analyzer
Incident Angle:	54.7°
Emission Angle:	0°
Analyzer Pass Energy:	160 eV
Analyzer Resolution:	1 eV
Total Signal Accumulation Time:	120 s
Total Elapsed Time:	Not specified
Number of Scans:	1
Effective Detector Width:	16 eV

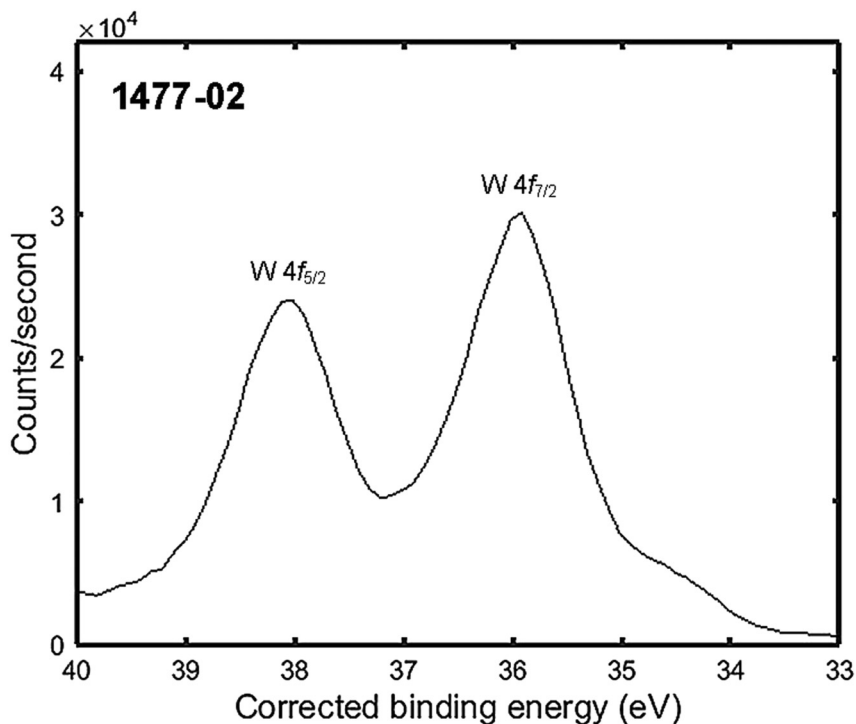


- Accession #: 01477-02
- Host Material: Ta₃N₅/W₁₈O₄₉ nanocomposite
- Technique: XPS
- Spectral Region: W 4f

Instrument: Kratos Axis Supra
 Excitation Source: Al K_α monochromatic
 Source Energy: 1486.6 eV
 Source Strength: 225 W
 Source Size: 0.7 mm × 0.3 mm
 Analyzer Type: Spherical sector
 Incident Angle: 54.7°
 Emission Angle: 0°
 Analyzer Pass Energy: 20 eV
 Analyzer Resolution: 0.1 eV
 Total Signal Accumulation Time: 17.75 s
 Total Elapsed Time: Not specified
 Number of Scans: 1
 Effective Detector Width: 2 eV

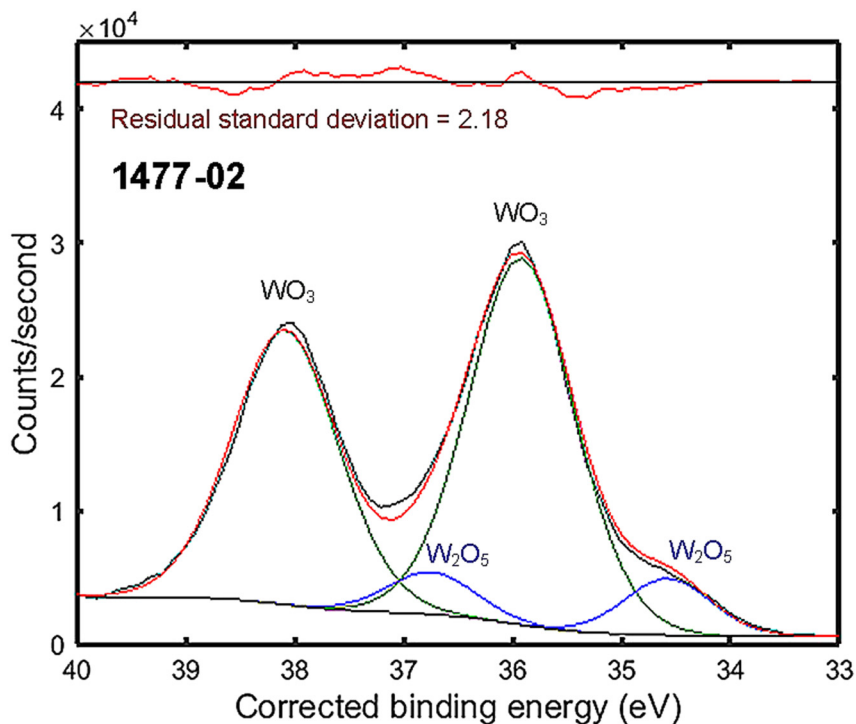


- Accession #: 01477-02
- Host Material: Ta₃N₅/W₁₈O₄₉ nanocomposite
- Technique: XPS
- Spectral Region: W 4f

Instrument: Kratos Axis Supra
 Excitation Source: Al K_α monochromatic
 Source Energy: 1486.6 eV
 Source Strength: 225 W
 Source Size: 0.7 mm × 0.3 mm
 Analyzer Type: Spherical sector
 Incident Angle: 54.7°
 Emission Angle: 0°
 Analyzer Pass Energy: 20 eV
 Analyzer Resolution: 0.1 eV
 Total Signal Accumulation Time: 17.75 s
 Total Elapsed Time: Not specified
 Number of Scans: 1
 Effective Detector Width: 2 eV

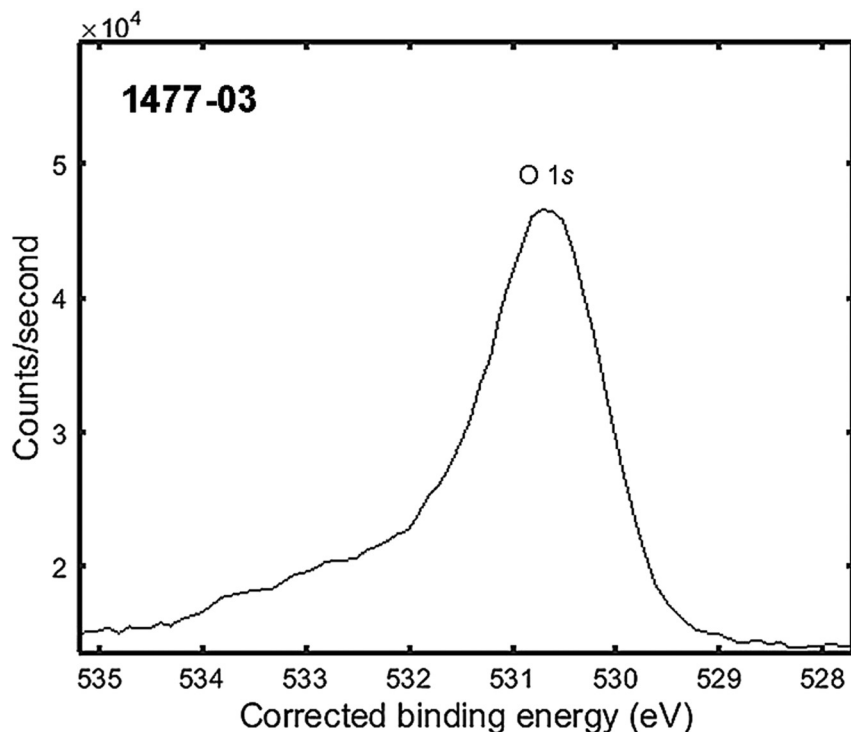


- Accession #: 01477-03
- Host Material: Ta₃N₅/W₁₈O₄₉ nanocomposite
- Technique: XPS
- Spectral Region: O 1s

Instrument: Kratos Axis Supra
 Excitation Source: Al K_α monochromatic
 Source Energy: 1486.6 eV
 Source Strength: 225 W
 Source Size: 0.7 mm × 0.3 mm
 Analyzer Type: Spherical sector
 Incident Angle: 54.7°
 Emission Angle: 0°
 Analyzer Pass Energy: 20 eV
 Analyzer Resolution: 0.1 eV
 Total Signal Accumulation Time: 19 s
 Total Elapsed Time: Not specified
 Number of Scans: 1
 Effective Detector Width: 2 eV

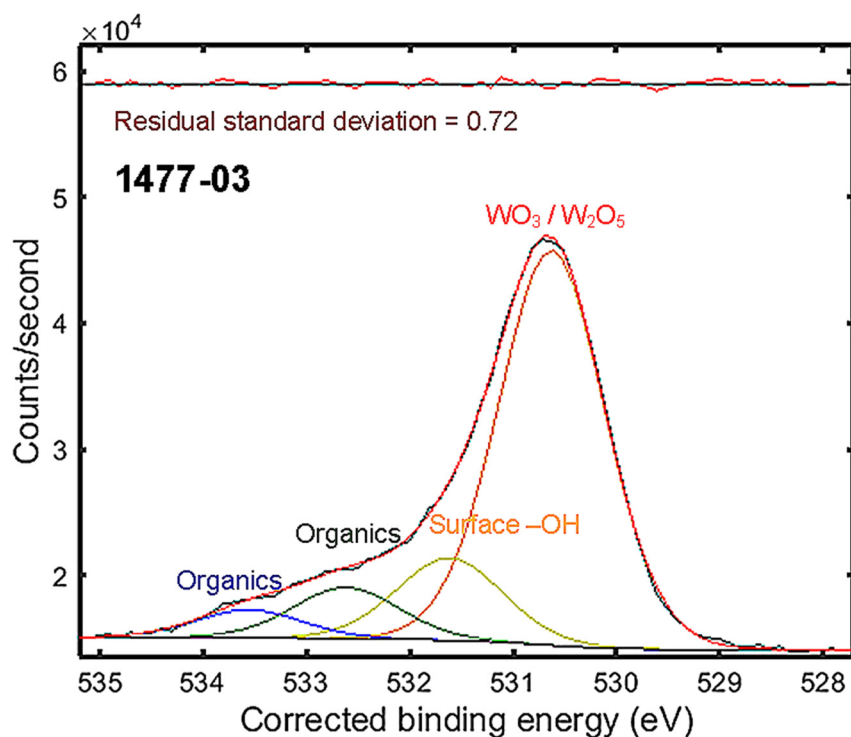


- Accession #: 01477-03
- Host Material: Ta₃N₅/W₁₈O₄₉ nanocomposite
- Technique: XPS
- Spectral Region: O 1s

Instrument: Kratos Axis Supra
 Excitation Source: Al K_α monochromatic
 Source Energy: 1486.6 eV
 Source Strength: 225 W
 Source Size: 0.7 mm × 0.3 mm
 Analyzer Type: Spherical sector
 Incident Angle: 54.7°
 Emission Angle: 0°
 Analyzer Pass Energy: 20 eV
 Analyzer Resolution: 0.1 eV
 Total Signal Accumulation Time: 19 s
 Total Elapsed Time: Not specified
 Number of Scans: 1
 Effective Detector Width: 2 eV

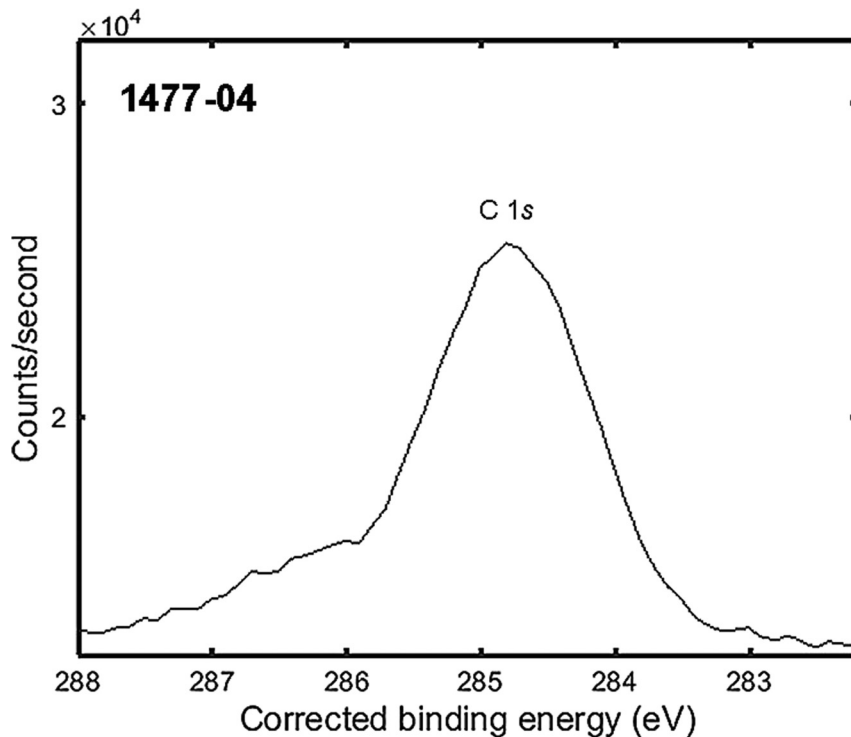


- Accession #: 01477-04
- Host Material: Ta₃N₅/W₁₈O₄₉ nanocomposite
- Technique: XPS
- Spectral Region: C 1s

Instrument: Kratos Axis Supra
 Excitation Source: Al K_α monochromatic
 Source Energy: 1486.6 eV
 Source Strength: 225 W
 Source Size: 0.7 mm × 0.3 mm
 Analyzer Type: Spherical sector
 Incident Angle: 54.7°
 Emission Angle: 0°
 Analyzer Pass Energy: 20 eV
 Analyzer Resolution: 0.1 eV
 Total Signal Accumulation Time: 29.5 s
 Total Elapsed Time: Not specified
 Number of Scans: 2
 Effective Detector Width: 2 eV

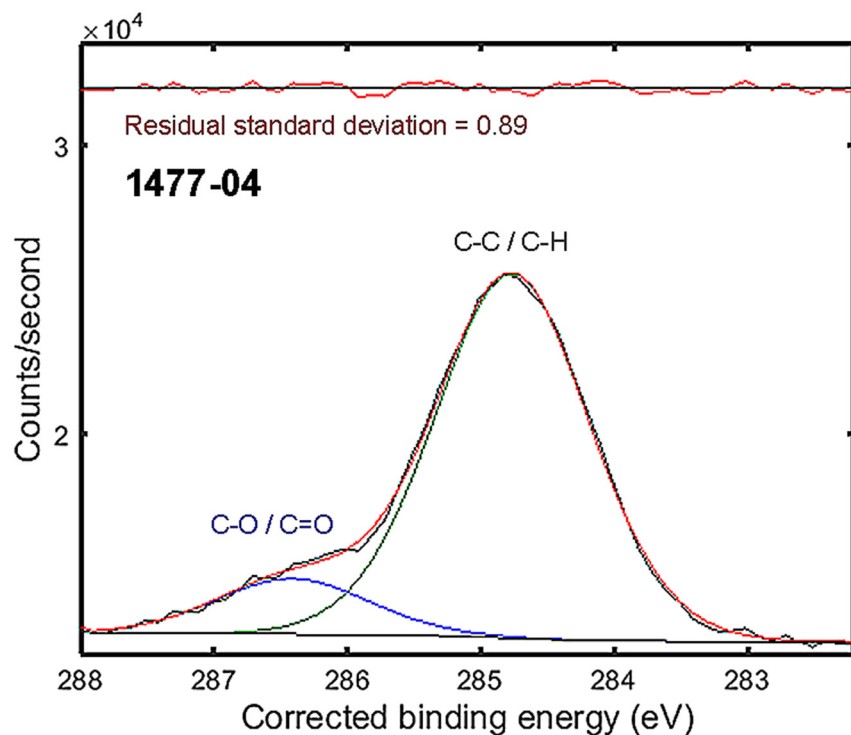


- Accession #: 01477-04
- Host Material: Ta₃N₅/W₁₈O₄₉ nanocomposite
- Technique: XPS
- Spectral Region: C 1s

Instrument: Kratos Axis Supra
 Excitation Source: Al K_α monochromatic
 Source Energy: 1486.6 eV
 Source Strength: 225 W
 Source Size: 0.7 mm × 0.3 mm
 Analyzer Type: Spherical sector
 Incident Angle: 54.7°
 Emission Angle: 0°
 Analyzer Pass Energy: 20 eV
 Analyzer Resolution: 0.1 eV
 Total Signal Accumulation Time: 29.5 s
 Total Elapsed Time: Not specified
 Number of Scans: 2
 Effective Detector Width: 2 eV

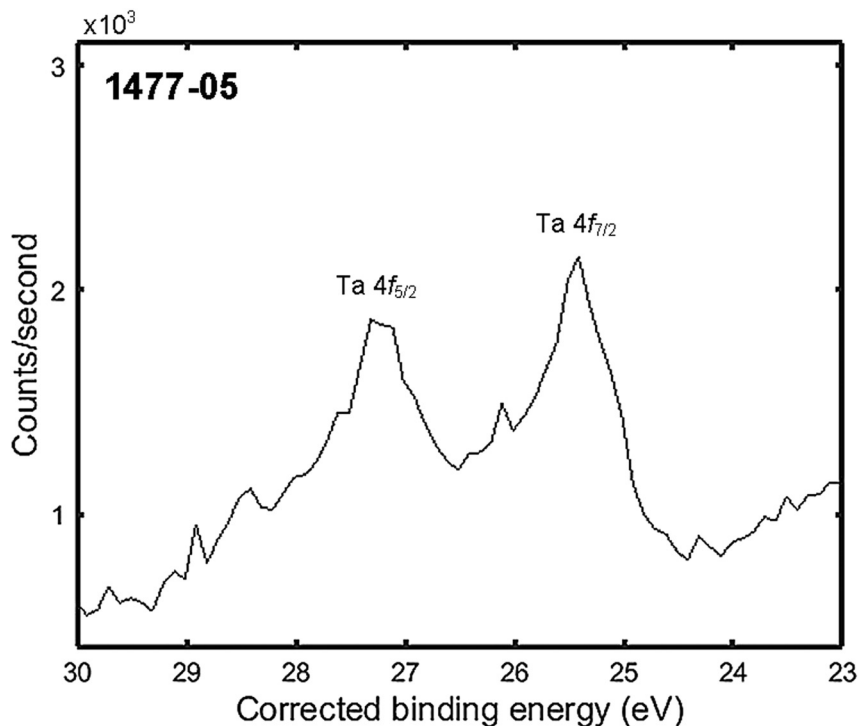

- Accession #: [01477-05](#)
- Host Material: Ta₃N₅/W₁₈O₄₉ nanocomposite
- Technique: XPS
- Spectral Region: Ta 4f

Instrument: Kratos Axis Supra
 Excitation Source: Al K_α monochromatic
 Source Energy: 1486.6 eV
 Source Strength: 225 W
 Source Size: 0.7 mm × 0.3 mm
 Analyzer Type: Spherical sector
 Incident Angle: 54.7°
 Emission Angle: 0°
 Analyzer Pass Energy: 20 eV
 Analyzer Resolution: 0.1 eV
 Total Signal Accumulation Time: 17.5 s
 Total Elapsed Time: Not specified
 Number of Scans: 1
 Effective Detector Width: 2 eV

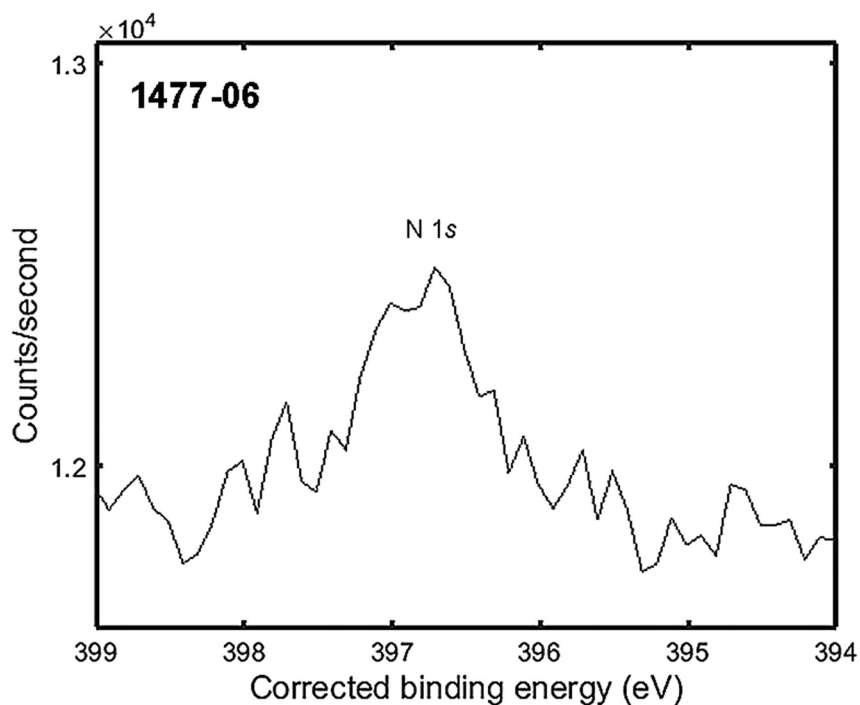

- Accession #: [01477-06](#)
- Host Material: Ta₃N₅/W₁₈O₄₉ nanocomposite
- Technique: XPS
- Spectral Region: N 1s

Instrument: Kratos Axis Supra
 Excitation Source: Al K_α monochromatic
 Source Energy: 1486.6 eV
 Source Strength: 225 W
 Source Size: 0.7 mm × 0.3 mm
 Analyzer Type: Spherical sector
 Incident Angle: 54.7°
 Emission Angle: 0°
 Analyzer Pass Energy: 20 eV
 Analyzer Resolution: 0.1 eV
 Total Signal Accumulation Time: 62.5 s
 Total Elapsed Time: Not specified
 Number of Scans: 5
 Effective Detector Width: 2 eV